


Basic samples

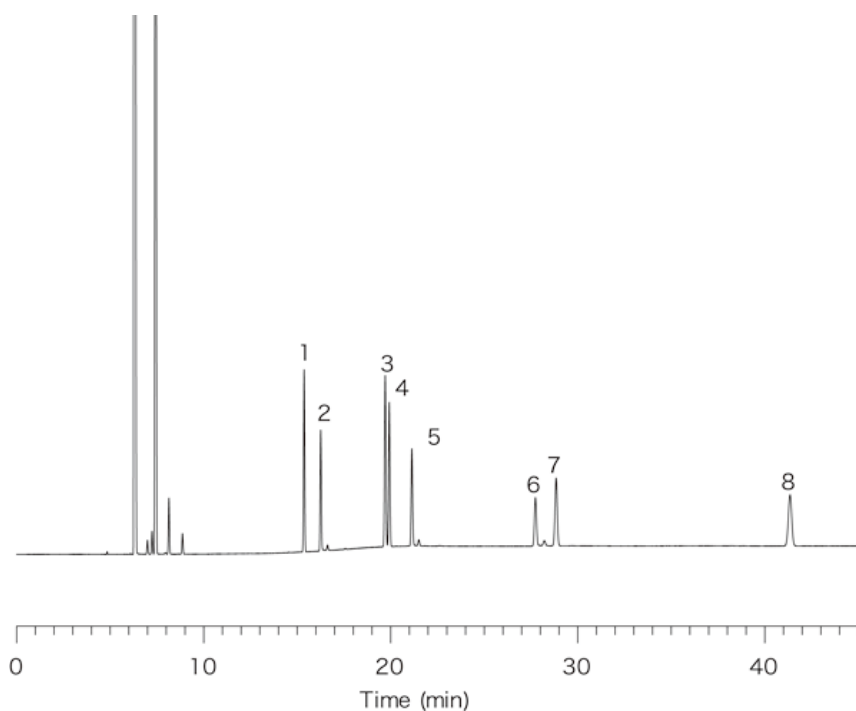

System : GC/FID
 Column : InertCap for Amines
 0.32mm I.D. × 60m
 Column Temp. : 100°C → 10°C/min → 250°C (30min)
 Carrier Gas : He 150kPa
 Injection : Split 1 : 50
 Detection : FID
 Sample : Basic amines, Hydrocarbons

Solutes : 1. n-Decane
 2. Amino octane
 3. 2,6-Dimethylaniline
 4. n-Dodecane
 5. 1-Amino decane
 6. Dicyclohexylamine
 7. 1-Amino dodecane
 8. n-Heptadecane