


# Organic solvents

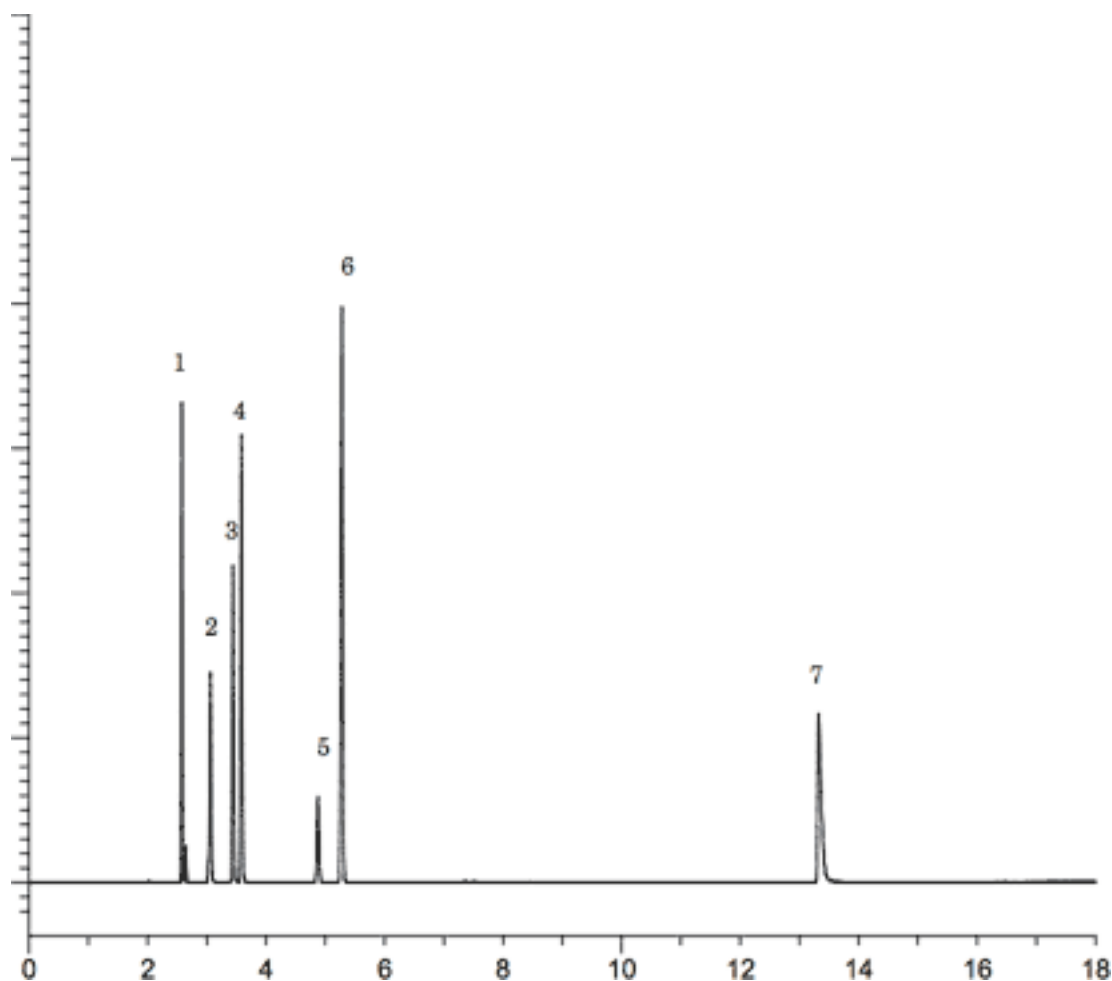

System	: GC/FID	Solutes	: 1. Acetone
Column	: InertCap Pure-WAX 0.25mmI.D. × 30m		2. Methanol
Column Temp.	df=0.25µm		3. Ethanol
Carrier Gas	: 50°C(5min)→10°C/min→250°C		4. Benzene
Injection	: He 100kPa		5. Chloroform
	: Split 1 : 80 0.1µl		6. Toluene
Detection	250°C		7. Acetic acid
	: FID Range 10 <sup>0</sup>		
Sample	260°C		
	: Organic solents		