


# Organic solvents

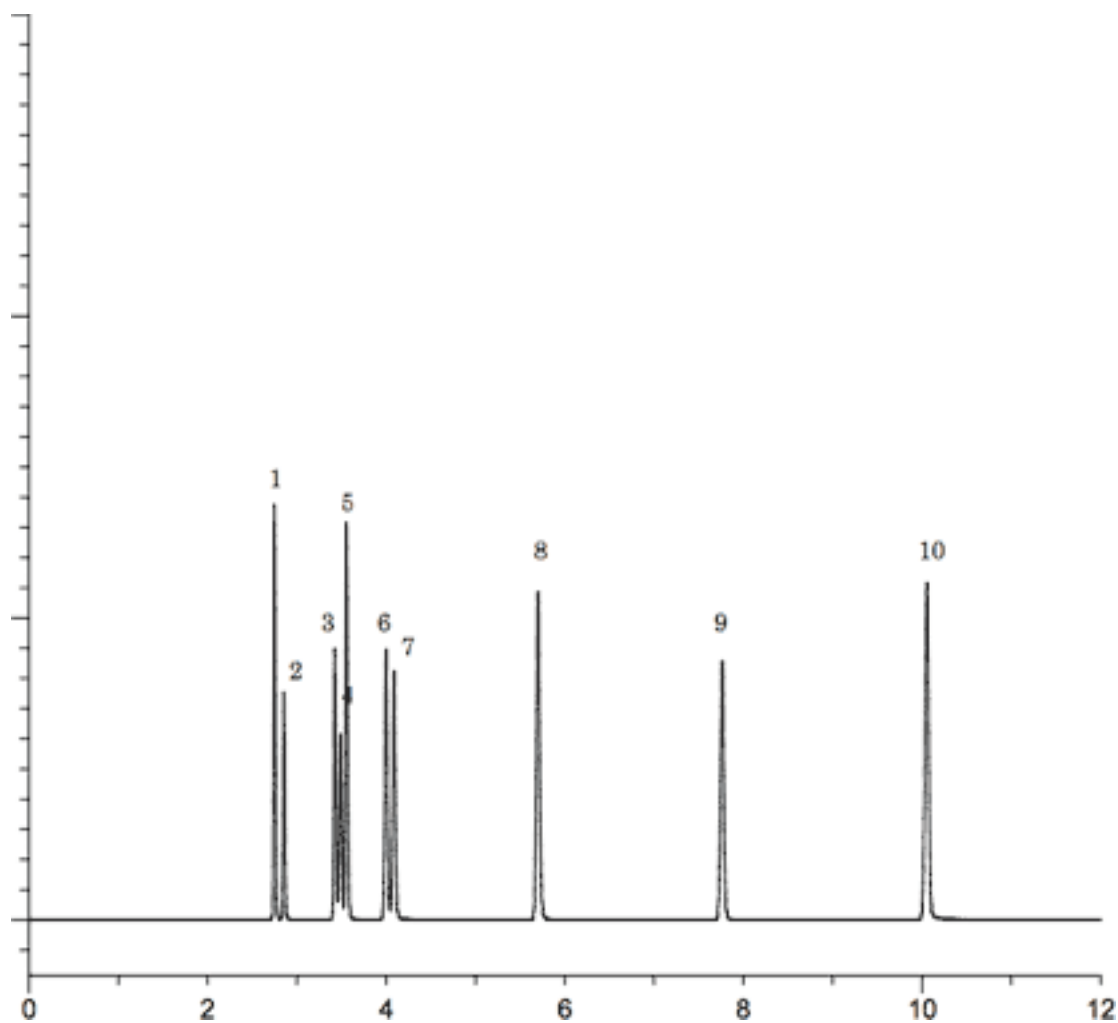

System	: GC/FID	Solutes	: 1. Acetone
Column	: InertCap Pure-WAX 0.25mmI.D. × 30m df=0.25µm		2. Methyl acetate
Column Temp.	: 40°C(min)→5°C/min→100°C		3. Ethyl acetate
Carrier Gas	: He 100kPa		4. Methanol
Injection	: Split 1 : 80 0.1µl 250°C		5. Methyl ethyl ketone
Detection	: FID Range 10 <sup>0</sup> 260°C		6. iso-Propanol
Sample	: Organic solents		7. Ethanol
			8. Methyl isobutyl ketone
			9. n-Butyl acetate
			10. n-Butanol