


Flavor by Japanese Standards of Food Additives

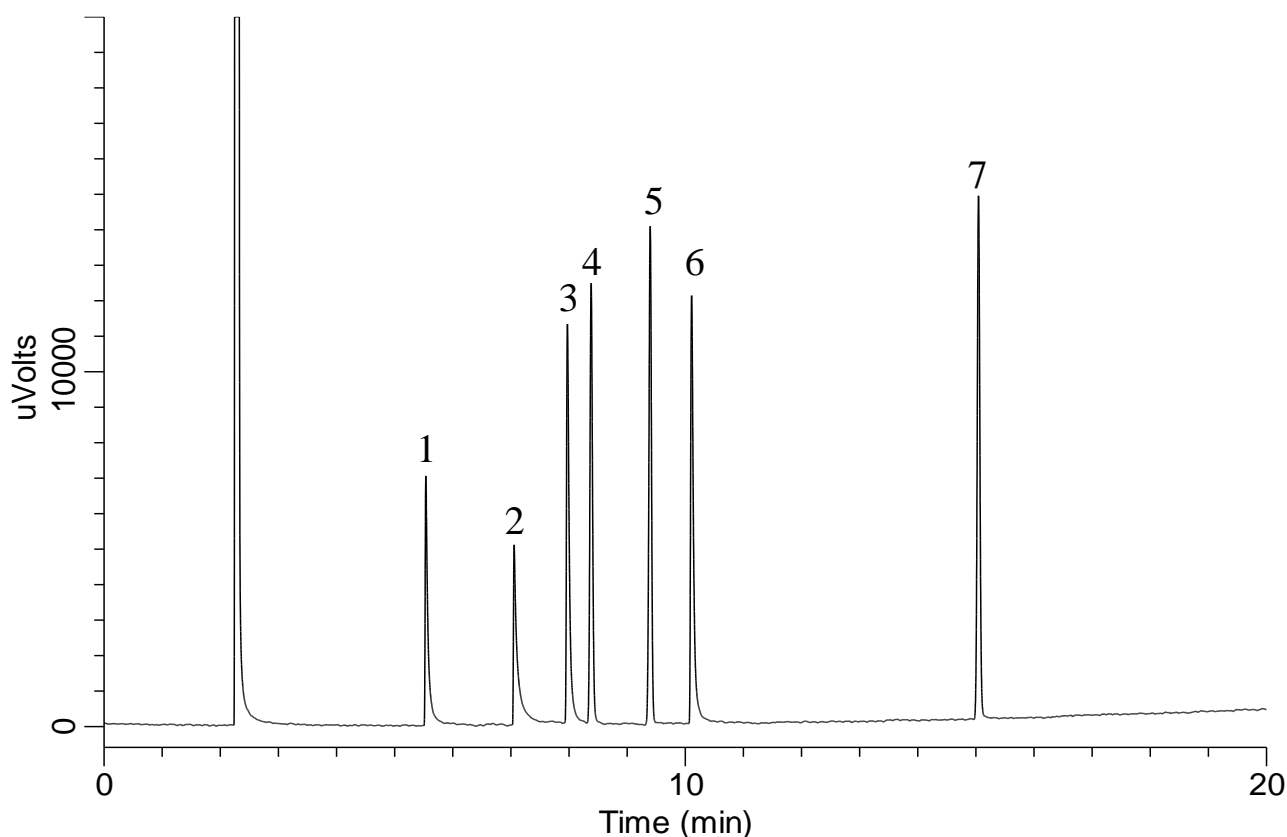

Conditions

System : GC-FID
Column : InertCap 1
 0.25 mm I.D. × 30 m df = 1.00 μm
Col. Cat. No. : 1010-11145
Col. Temp. : 50 °C(5 min hold) - 5 °C/min - 230 °C
Carrier Gas : He 100 kPa
Injection : Split flow 360 mL/min
 250 °C
Detection : FID Auto Range
 250 °C
Sample Size : 1000 μg/mL in Methanol
 1 μL

Analyte

1. Butylamine
 2. Pyrrolidine
 3. Isopentylamine
 4. Pyrazine
 5. Pyrrole
 6. Piperidine
 7. 2,6-Dimethylpyridine