


Flavor by Japanese Standards of Food Additives

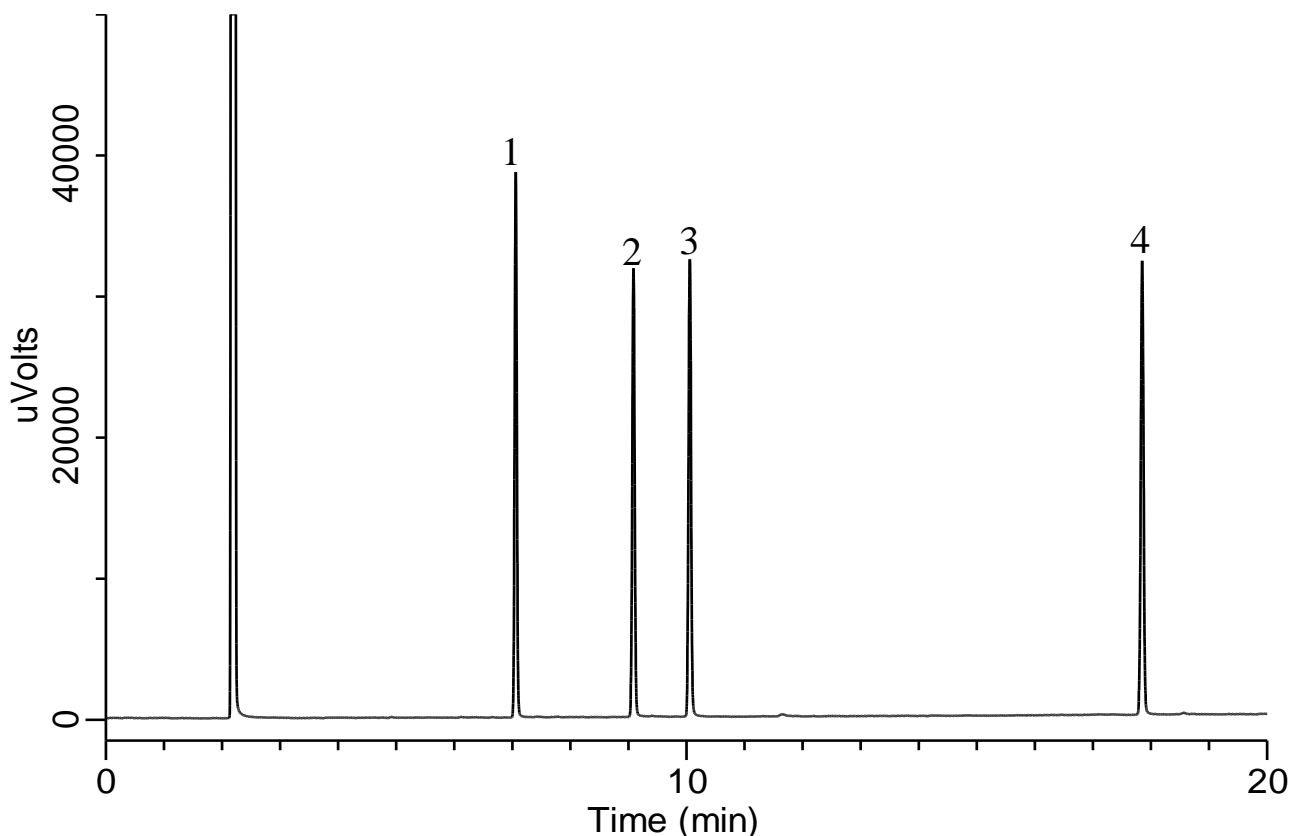

Conditions

System : GC-FID
Column : InertCap 1
 0.25 mm I.D. × 30 m df = 0.25 μm
Col. Cat. No. : 1010-11142
Col. Temp. : 100 °C - 5 °C/min - 230 °C
Carrier Gas : He 80 kPa
Injection : Split flow 120 mL/min
 250 °C
Detection : FID Auto Range
 250 °C
Sample Size : 1000 μg/mL in Methanol
 1 μL

Analyte

1. 5,6,7,8-Tetrahydroquinoxaline
 2. 5-Methylquinoxaline
 3. 6-Methylquinoline
 4. 2-(3-Phenylpropyl)pyridine