


Analysis of Clofibrate

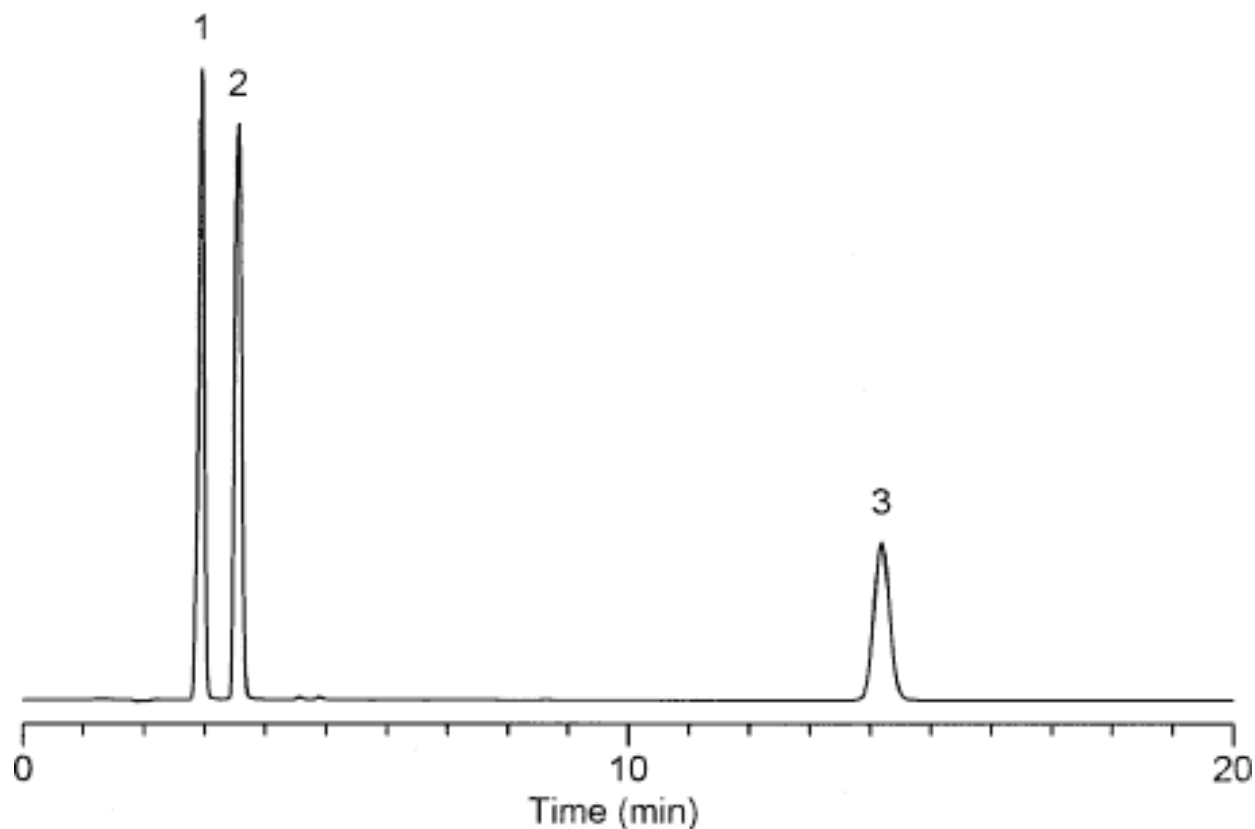

Column	:Inertsil ODS-3V 5µm 250 × 4.6mmI.D.	Solutes	: 1. p-Ethoxyphenol 2.953 2. p-Chlorophenol 3.563 3. Clofibrate 14.180
Column Cat. No. :			
Eluent	:acetonitrile / 0.1% phosphoric acid=60/40		
Flow rate	:1.5 mL/min.		
Col. Temp.	:25°C		
Detection	:UV 275 nm		
Injection Vol.	:10µL		
Sample	:Clofibrate (1mg/mL) p-Chlorophenol (0.6mg/mL) p-Ethoxyphenol (0.6mg/mL)		