


Analysis of DNPH-Aldehydes

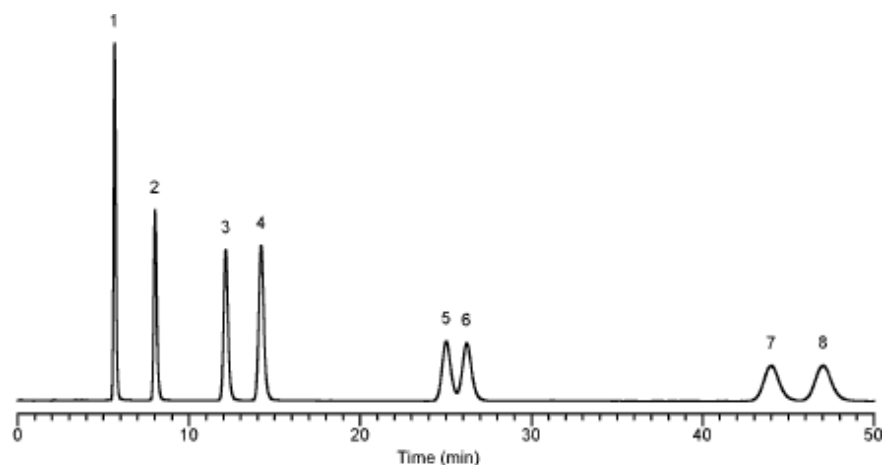

No.	Peak Name	R.Time	Area
1	Formaldehyde	5.640	519500
2	Acetaldehyde	8.013	382328
3	Acetone	12.133	432589
4	Propionaldehyde	14.203	517848
5	n-Butyraldehyde	25.017	339450
6	iso-Butyraldehyde	26.213	352575
7	iso-Valeraldehyde	43.993	340633
8	n-Valeraldehyde	47.033	360519

Column : Inertsil C4
5 μ m
150 \times 4.6 mmI.D.

Column Cat. No. : 5020-01401

Eluent : CH₃OH/H₂O = 48/52

Flow rate : 1.0 mL/min.

Col. Temp. : 40°C

Detection : UV 360 nm

Injection Vol. : 1 μ L

Sample :

Solutes : 1. DNPH-Formaldehyde (0.1mg/mL)
2. DNPH-Acetaldehyde (0.1mg/mL)
3. DNPH-Acetone (0.1mg/mL)
4. DNPH-Propionaldehyde (0.1mg/mL)
5. DNPH-n-Butyraldehyde (0.1mg/mL)
6. DNPH-iso-Butyraldehyde (0.1mg/mL)
7. DNPH-iso-Valeraldehyde (0.1mg/mL)
8. DNPH-n-Valeraldehyde (0.1mg/mL)