


Anions

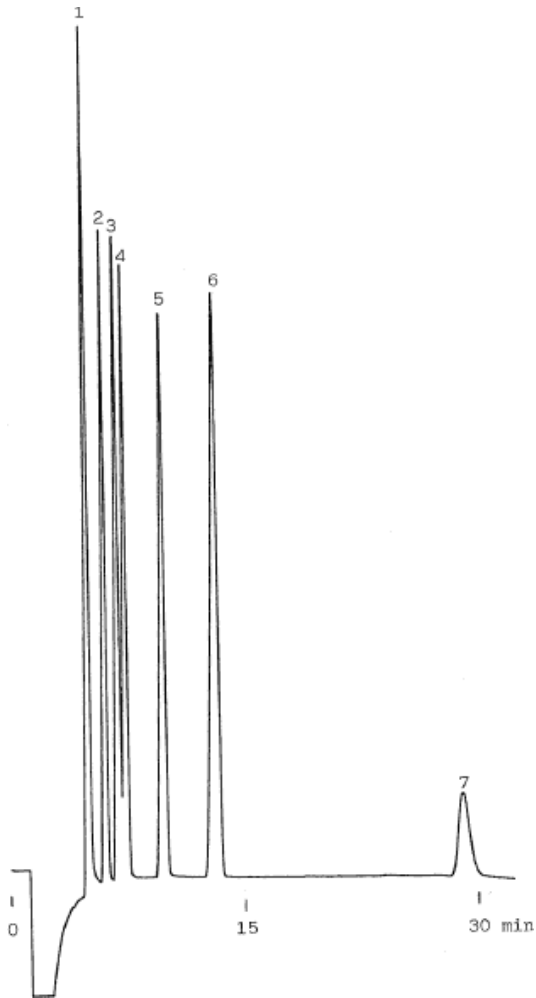

Column : Inertsil C4
 5µm
 150 × 4.6 mm I.D.

Column Cat. No. : 5020-01401

Eluent : 1 mM IPCA-03H + 0.5 mM Phthalic acid

Flow rate : 1.0 mL/min.

Col. Temp. : 40°C

Detection : UV 254 nm

Injection Vol. :

Sample : Inorganic anion

Solutes : 1. F-
 2. Cl-
 3. Br-
 4. NO₂-
 5. NO₃-
 6. ClO₃-
 7. SO₄²⁻