


# Anions in Tap water

Data No. LA424-0000

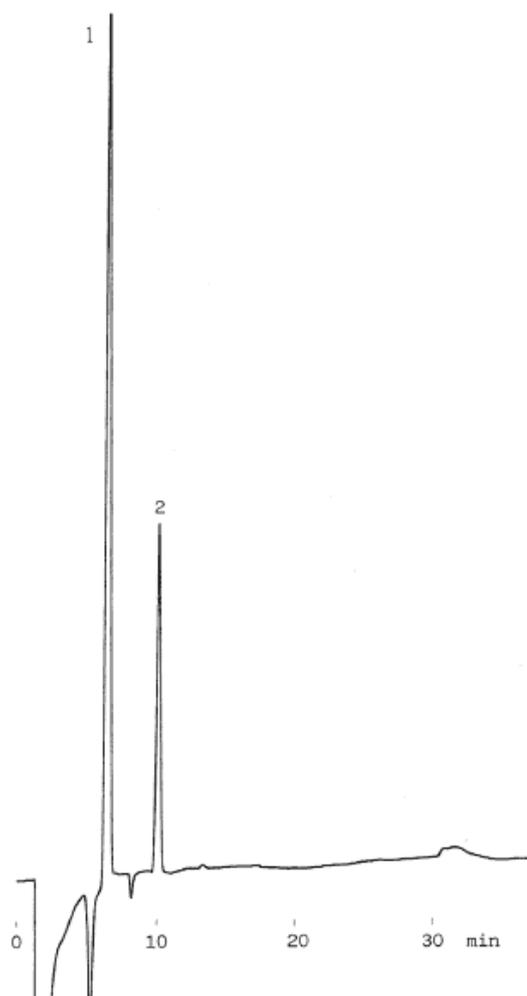

Column : Inertsil C4  
5 $\mu$ m  
150  $\times$  4.6 mm I.D.

Solutes : 1. Cl-  
2. NO<sub>3</sub>-

Column Cat. No. : 5020-01401

Eluent : 1 mM IPCA-03H + 0.5 mM Phthalic acid  
IPCA-03H: Tetra-n-butylammonium Hydroxide

Flow rate : 1.0 mL/min.

Col. Temp. : 40°C

Detection : UV 254 nm

Injection Vol. :

Sample : Inorganic anion