


Analysis of Samples for Column Selectivity

Data No. LA439-0000

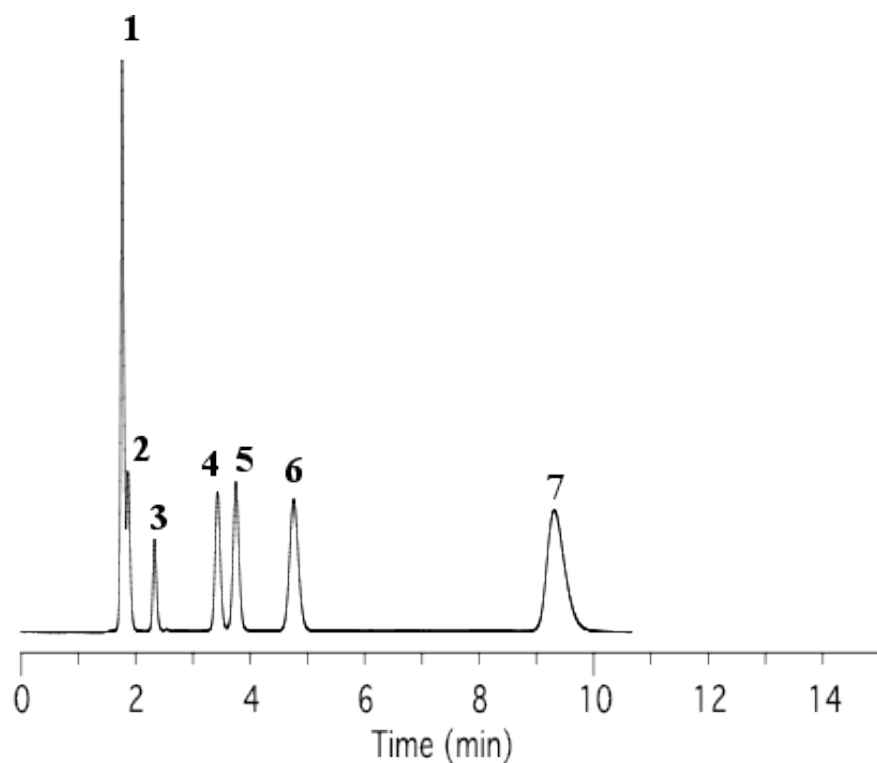

Column : Inertsil CN-3
5 µm
150 x 4.6 mm I.D.

Column Cat. No. : 5020-01940

Eluent : A) CH₃OH
B) H₂O
A/B = 60/40, v/v

Flow rate : 1.0 mL/min.

Col. Temp. : 40°C

Detection : UV 254 nm

Injection Vol. :

Sample :

Solutes : 1. Uracil
2. Caffeine
3. Phenol
4. n-Butylbenzene
5. n-Amylbenzene
6. o-Terphenyl
7. Triphenylene