


Analysis of Samples for Column Selectivity

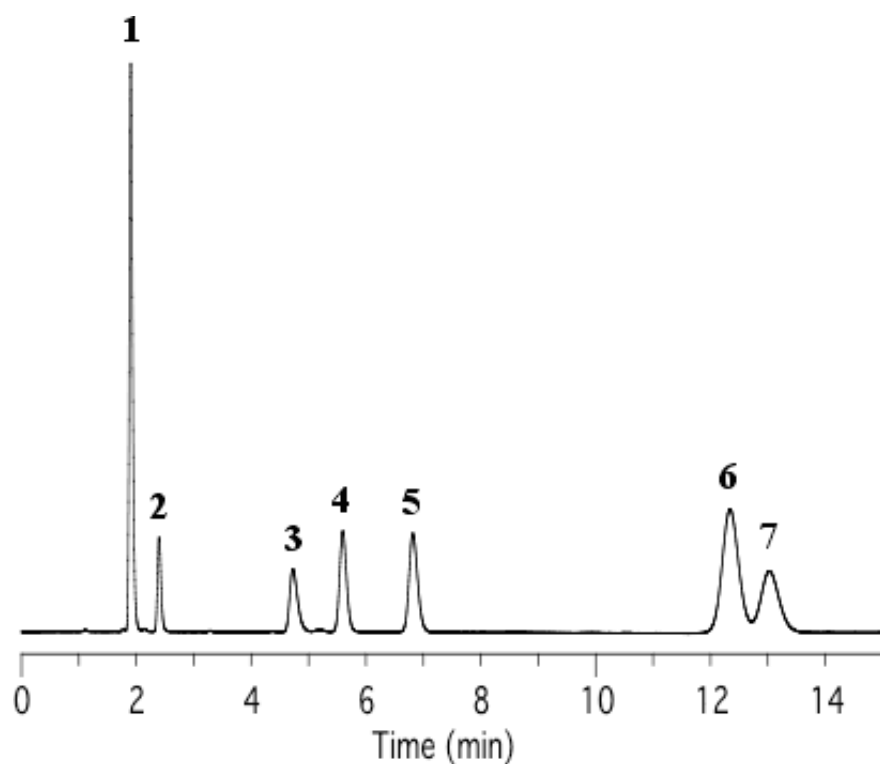

Column : Inertsil Ph-3
5 μm
150 x 4.6 mm I.D.

Column Cat. No. : 5020-01302

Eluent : A) CH₃OH
B) H₂O
A/B = 60/40, v/v

Flow rate : 1.0 mL/min.

Col. Temp. : 40°C

Detection : UV 254 nm

Injection Vol. :

Sample :

Solutes : 1. Uracil
2. Phenol
3. Caffeine
4. n-Butylbenzene
5. n-Amylbenzene
6. Triphenylene
7. o-Terphenyl