


Analysis of nucleotide

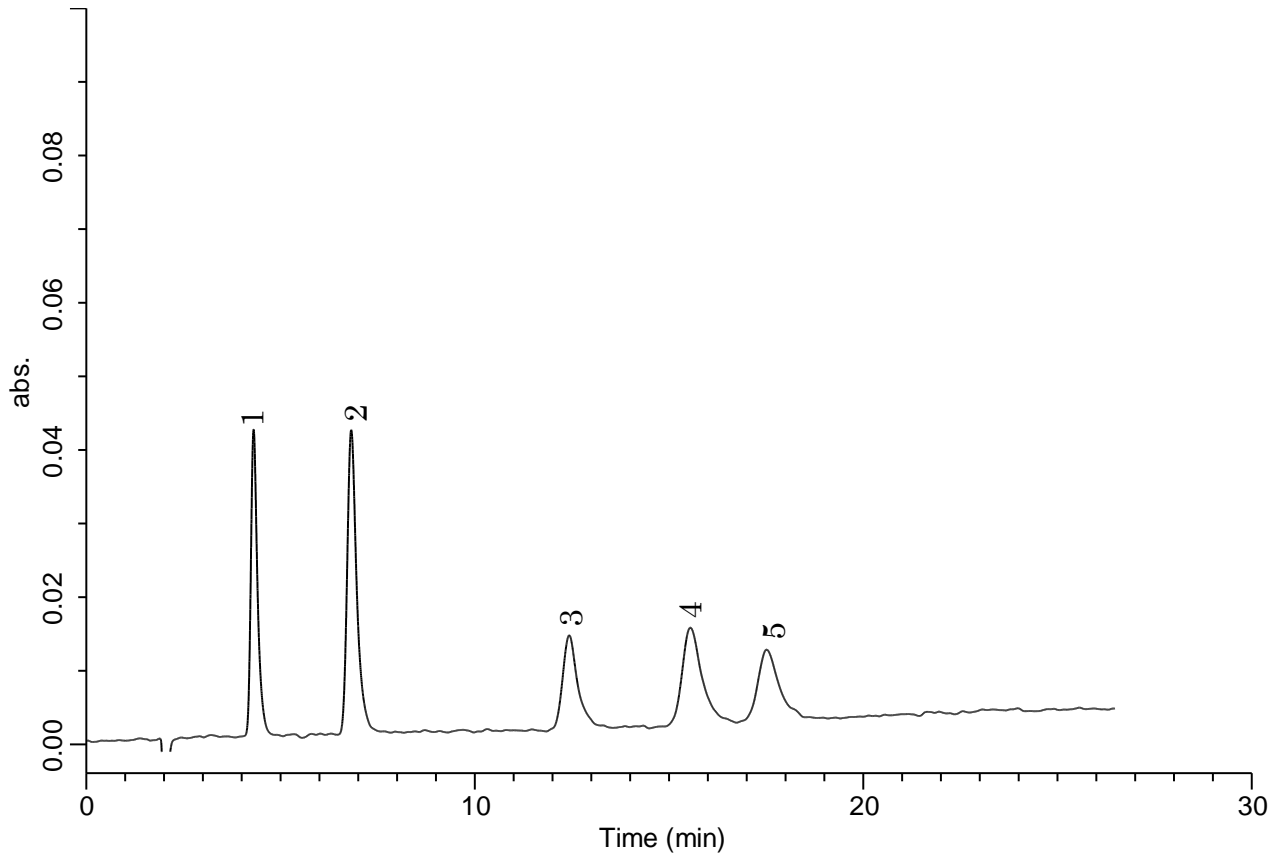

Conditions

System : GL-7400 HPLC system
Column : Inertsil NH2 (5 μ m, 150 x 4.6 mm I.D.)
Column Cat. No. : 5020-05545
Eluent : A) CH₃OH
 : B) 20 mM KH₂PO₄ (pH 2.03, H₃PO₄)
 : A/B = 50/50, v/v
Flow rate : 1.0 mL/min
Col. Temp. : 40 °C
Detection : UV 260 nm (GL-7450 UV Detector)
Injection Vol. : 10 μ L
Sample : nucleotide

Analyte:

1. 5'-CMP (40 mg/L)
 2. 5'-AMP (40 mg/L)
 3. 5'-UMP (40 mg/L)
 4. 5'-GMP (40 mg/L)
 5. 5'-IMP (40 mg/L)