


Analysis of Aromatic carboxylic acids

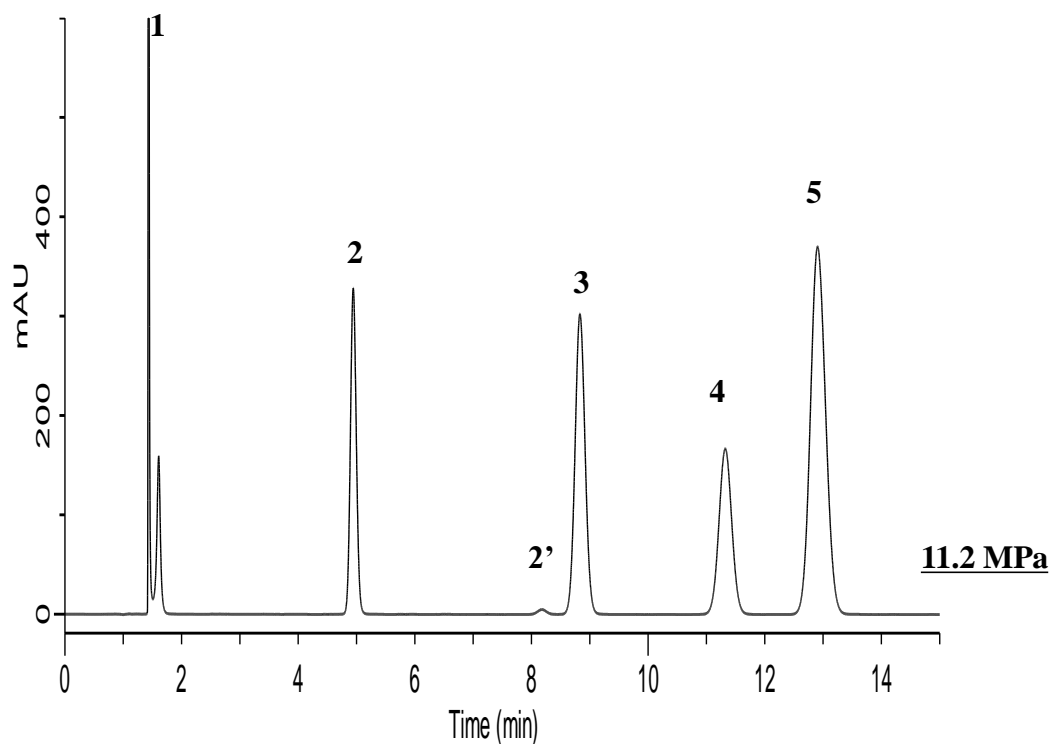

Conditions

System : GL-7400 system
Column : Inertsil ODS-3 (3 μm , 100 x 4.6 mm I.D.)
Column Cat. No. : 5020-01775
Eluent : A) CH_3CN
 B) 0.1 % H_3PO_4
 A/B = 15/85, v/v
Flow Rate : 1.0 mL/min
Col. Temp. : 40 $^\circ\text{C}$
Detector : UV 275 nm (GL-7452A PDA Detector)
Injection Vol. : 10 μL

Analyte

1. Gallic acid	(0.17 mg/mL)
2. Vanillic acid	(0.17 mg/mL)
2' Vanillin	(Impurity of 2)
3. <i>p</i> -Coumaric acid	(0.17 mg/mL)
4. Ferulic acid	(0.17 mg/mL)
5. <i>m</i> -Coumaric acid	(0.17 mg/mL)