


Analysis of Glycyrrhiza

(Under the Condition of the Japanese Pharmacopoeia)

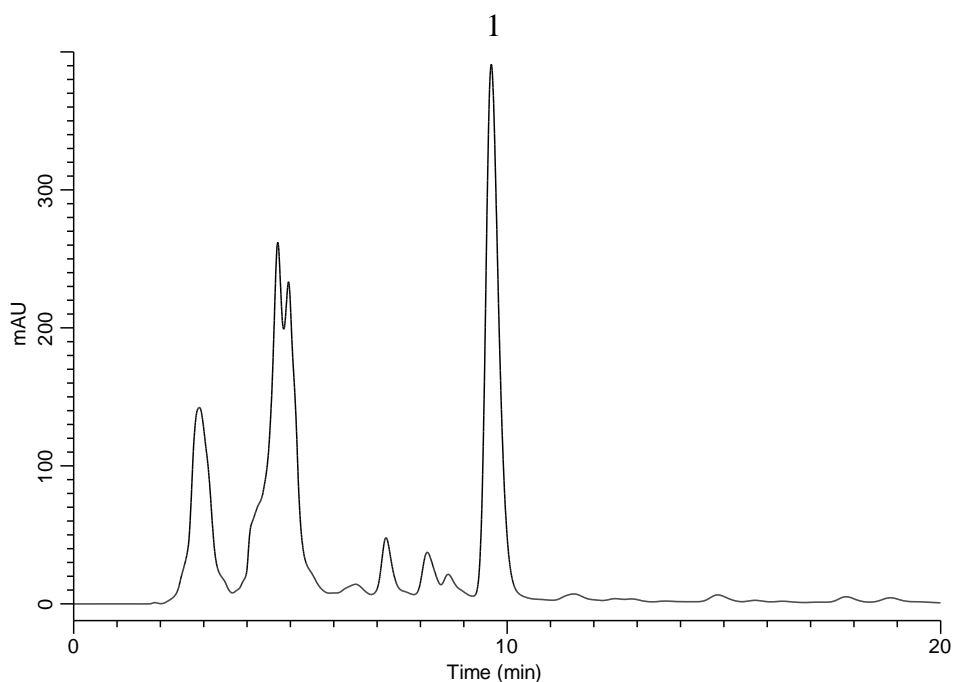

Conditions

System : GL-7400 HPLC system
Column : InertSustain C18
 (5 μ m, 150 x 4.6 mm I.D.)
Column Cat. No. : 5020-07345
Eluent : A) CH₃CN
 B) 2.1% CH₃COOH in H₂O
 A/B = 40/60, v/v
Flow Rate : 0.45 mL/min
Col. Temp. : 20 °C
Detection : UV 254 nm (GL-7452 PDA Detector)
Injection Vol. : 20 μ L
Sample : Sample solution

Analyte:

1. Glycyrrhizic acid 5000 mg/L

RSD of the
 peak area (n=5) : 0.15 (\leq 1.5)