


## Analysis of Tocopherol

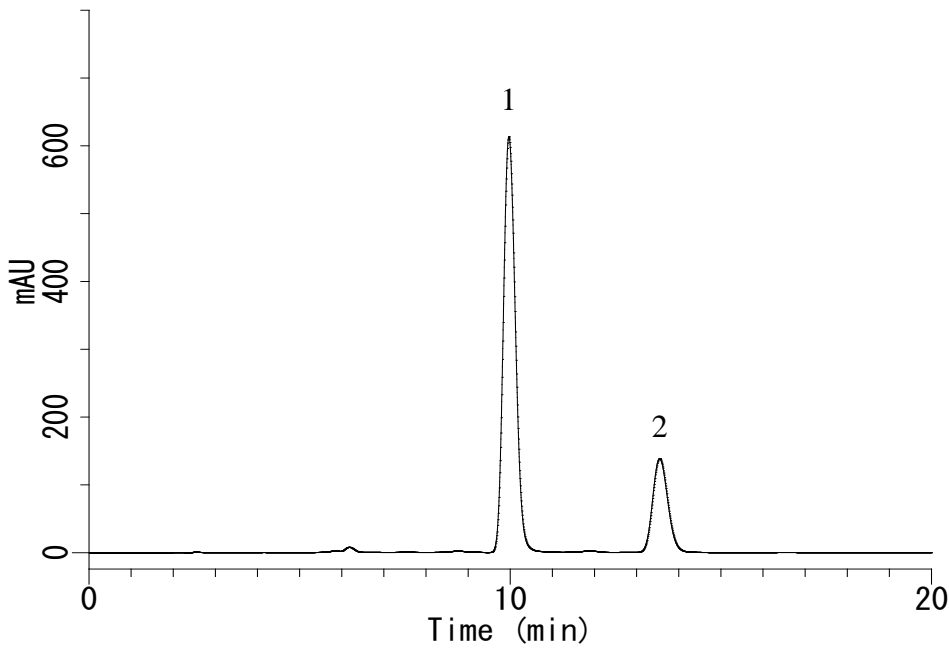

### Conditions

**System** : GL7700 HPLC system  
**Column** : Inertsil ODS-4  
 (5  $\mu$  m, 150 x 4.0 mm I.D.)  
**Column Cat. No.** : 5020-03935  
**Eluent** : A) CH<sub>3</sub>OH  
 B) H<sub>2</sub>O  
 A/B = 98/2, v/v  
**Flow Rate** : 0.62 mL/min  
**Col. Temp.** : 30 °C  
**Detection** : UV 292 nm (UV7750 UV Detector)  
**Injection Vol.** : 20  $\mu$  L  
**Sample** : Standard

### Analyte:

1. *d*- $\alpha$ -Tocopherol 1.0 mg/L  
 2. Tocopherol acetate 1.0 mg/L