


Analysis of Tocopherol

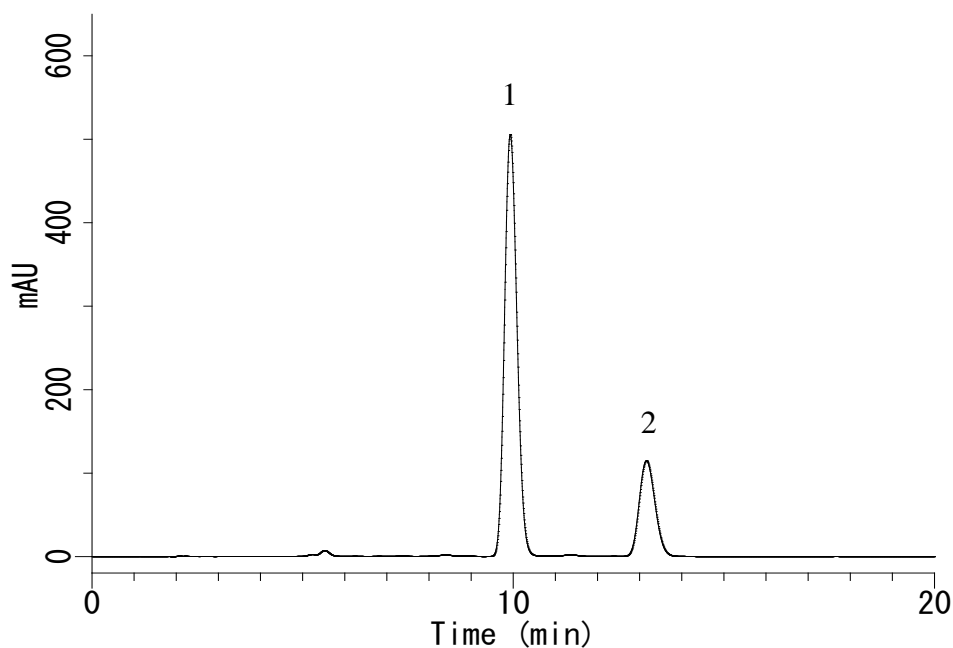

Conditions

System : GL7700 HPLC system
Column : Inertsil ODS-2
 (5 μ m, 150 x 4.0 mm I.D.)
Column Cat. No. : 5020-01123
Eluent : A) CH₃OH
 B) H₂O
 A/B = 98/2, v/v
Flow Rate : 0.73 mL/min
Col. Temp. : 30 °C
Detection : UV 292 nm (UV7750 UV Detector)
Injection Vol. : 20 μ L
Sample : Standard

Analyte:

1. *d*- α -Tocopherol 1.0 mg/L
 2. Tocopherol acetate 1.0 mg/L