


Analysis of Vitamin E

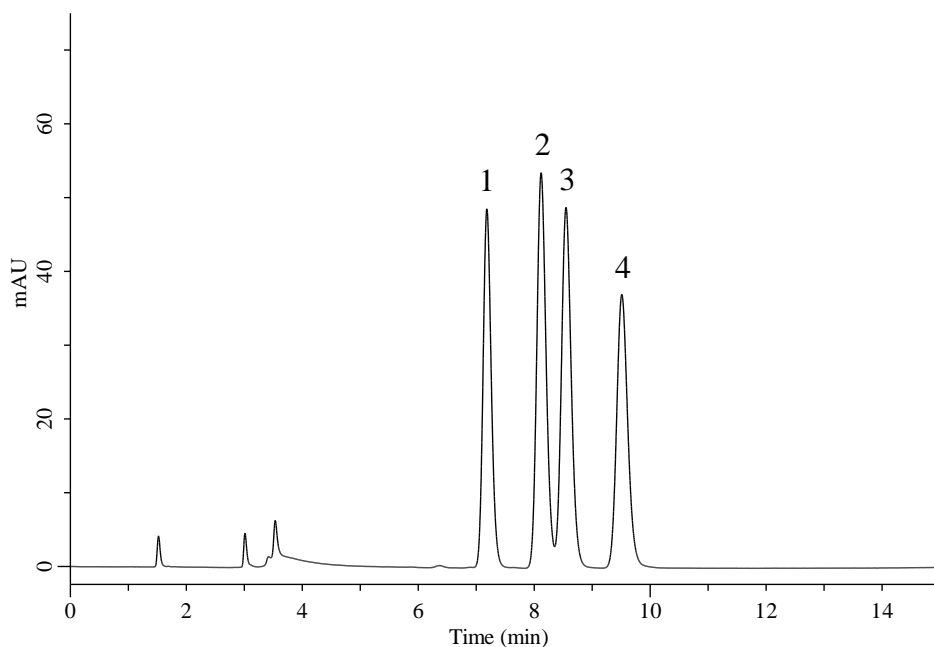

Conditions

System : Primaide HPLC system (HITACHI)
Column : InertSustain C30 (GL Sciences Inc.)
 (5 μ m, 250 x 4.6 mm I.D.)
Column Cat. No. : 5020-17145
Eluent : CH₃OH
Flow Rate : 1.0 mL/min
Col. Temp. : 25 °C
Detection : UV 210 nm
Injection Vol. : 5 μ L
Sample : Standard

Analyte:

1. δ -tocopherol
 2. γ -tocopherol
 3. β -tocopherol
 4. α -tocopherol
 (50 mg/L each)