


Analysis of Oligonucleotides

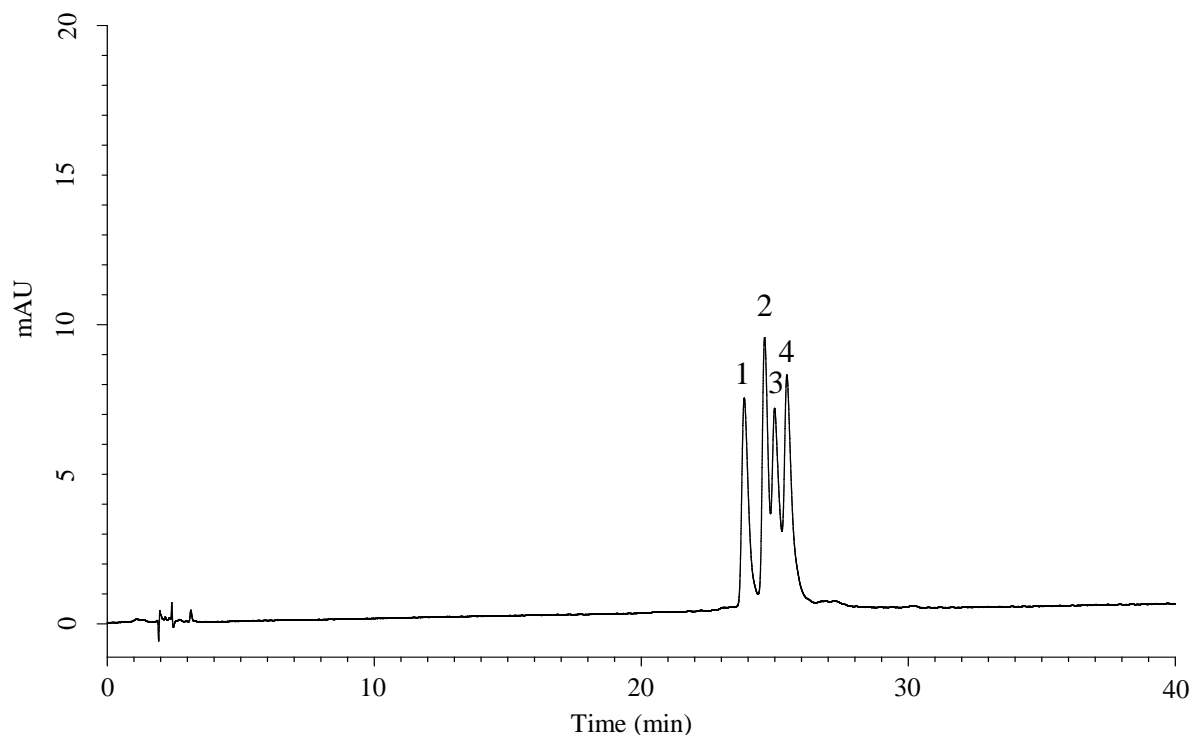

Conditions

Column : InertSustain AX-C18 (GL Sciences Inc.)
 (3 μ m, 150 x 2.1 mm I.D., Metal-free hardware)

Column Cat. No. : 5020-91059

Eluent : A) 200 mM HCOONH₄ in
 (CH₃CN/H₂O = 50/50, v/v)
 B) 200 mM HCOONH₄ in H₂O

Time (min)	A (vol%)	B (vol%)
0.0	10	90
40.0	30	70

Flow Rate : 0.2 mL/min

Col. Temp. : 40 °C

Detection : UV 260 nm

Injection Vol. : 2 μ L

Sample : Standard

Analyte:

1. 5'- CATGACGTTCTGATGCT-3' (18 mer)
2. 5'- TATGACGTTCTGATGCT-3' (18 mer)
3. 5'- GCTACGACGTTCTGATGCT-3' (20 mer)
4. 5'- GCTATGACGTTCTGATGCT-3' (20 mer)
 (10 mg/L each)