


Organic fluorine compounds

Specification
One GC Channel

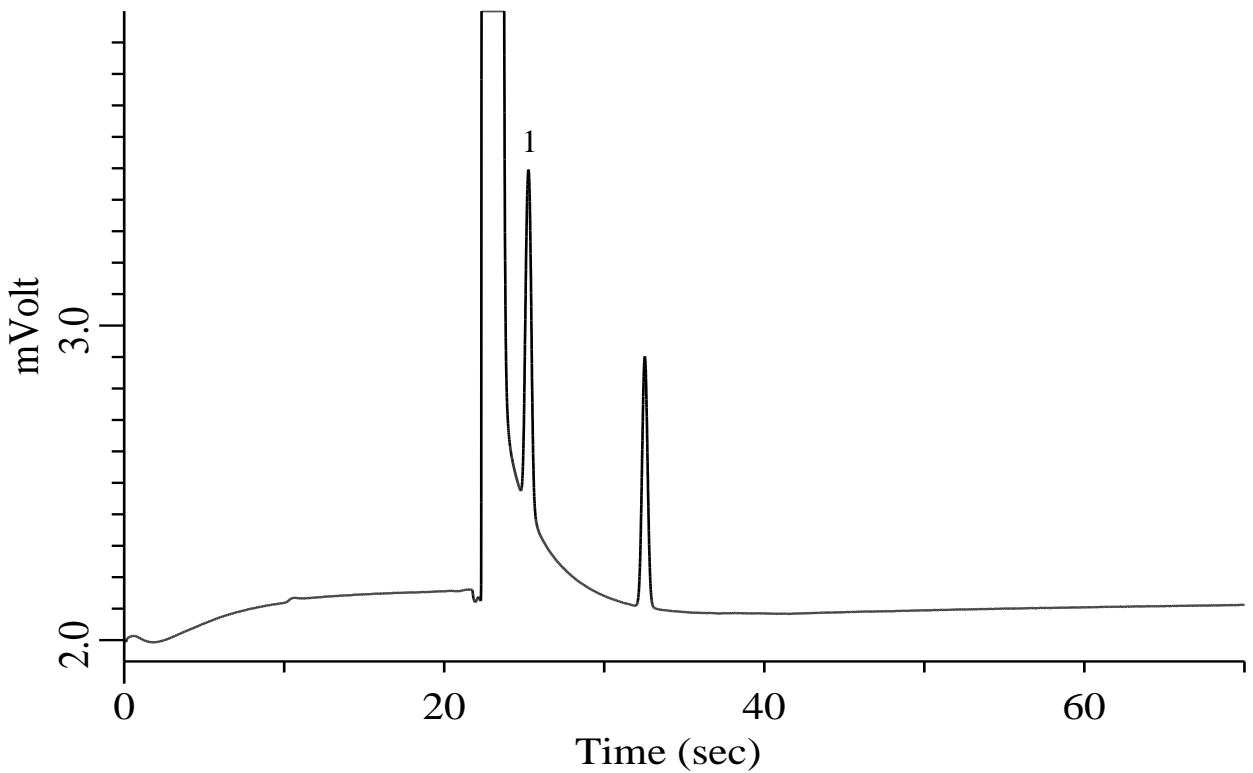

Conditions

System : Micro GC
 Column : PoraPLOT Q 10 m
 Column Temp. : 40 °C
 Carrier Gas : He 190 kPa
 Inject Time : 40 msec

Analyte:

1. Carbon tetrafluoride (R-14) 500 ppm (v/v)
 Balance Gas N₂